

APP'L	DATE	LVL	REVISION
DK	3/28/91	A	N0334
SCF	10/15/98	B	N0839
	10-04-11	C	N01413


## SPECIFICATIONS

### DEW POINT METER

POWER SUPPLY: 110v-1ph-50/60Hz  
 OPERATING TEMPERATURE: +32°F to +140°F  
 WARM-UP TIME: 3 minutes  
 OUTPUT: 4 to 20mA  
 ALARM: 2 alarm relays, one fault alarm relay,  
 and a single analog output.

### DEW POINT SENSOR

TYPE: Aluminum Oxide  
 CALIBRATED RANGE: -112°F to +68°F

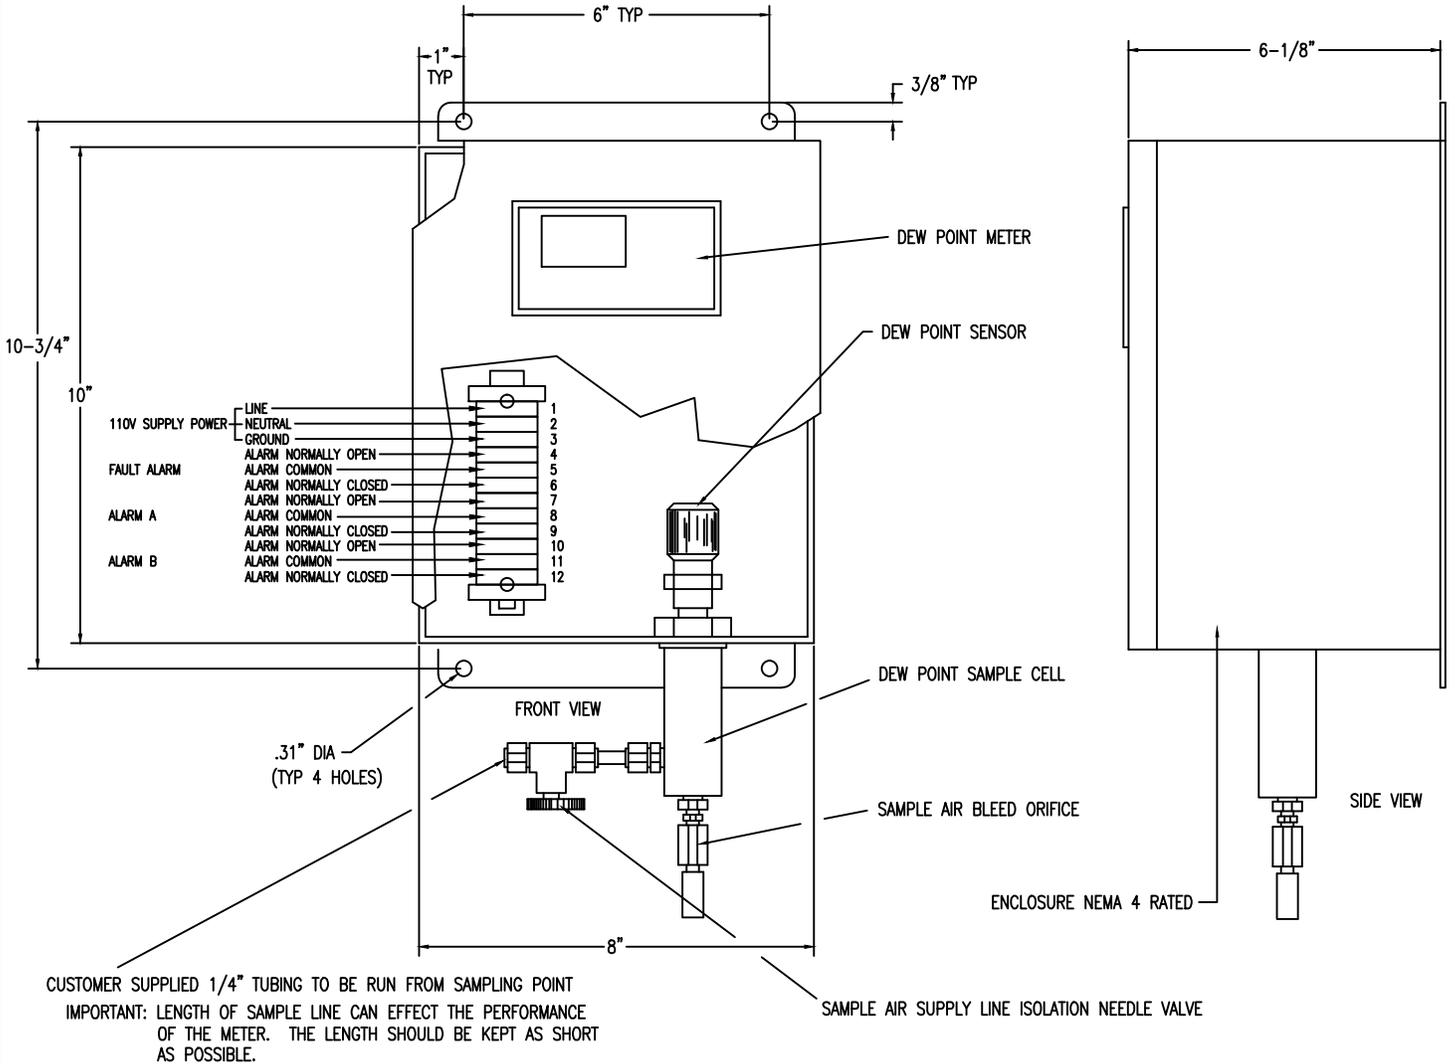

### INSTALLATION NOTES

- 1) Unit must be installed on a solid surface in a safe location free from possible damage.
- 2) Customer must supply and install all incoming power connections.
- 3) Customer must supply and install sample air supply line.
- 4) All alarm connections and/or applications are to be in accordance with manufacturer's Installation and Operation Instructions

This drawing is the property of

**VAN AIR SYSTEMS INC**

and is subject to return upon request. It shall not be copied or duplicated in any manner and shall not be submitted to outside parties for examination without the consent of Van Air Systems Inc. It shall be used for reference to work under contract or proposals submitted by Van Air Systems Inc. only.

DEW POINT METER ASSEMBLY

Part Number 81-1186

DRWN BY: JMK

DATE: 10-15-98

DRWG No. SD-12689

REV

CHECKED: SCF

SCALE: NONE

C

APPL: SCF

**VAN AIR SYSTEMS INC**

Lake City, PA 16423 (814)774-2631 Fax: 814/774-3482 Telex: 91-4548